



DIVISION OF INDUSTRY SERVICES
Plumbing Product Review
P.O. Box 2658
Madison, Wisconsin 53701-2658
TTY: Contact Through Relay

Scott Walker, Governor
Dave Ross, Secretary

March 28, 2016

MERCK KgaA
EMD MILLIPORE
MICHAEL PACEK
290 CONCORD ROAD
BILLERICA MA 01821

Re: Description: HEALTH CARE PLUMBING APPLIANCE
Manufacturer: MERCK KgaA
Product Name: (trans id) AFS WATER PURIFIERS FOR CLINICAL ANALYZERS
Model Number(s): 8, 16, 24, 10E, 15E, 40E, 80E, 120E AND 150E
Product File No: 20160105

The specifications and/or plans for this plumbing product have been reviewed and determined to be in compliance with chapters SPS 382 through 384, Wisconsin Administrative Code, and Chapters 145 and 160, Wisconsin Statutes.


The Department hereby issues an approval based on the Wisconsin Statutes and the Wisconsin Administrative Code. This approval is valid until the end of March 2021.

This approval is contingent upon compliance with the following stipulation(s):

- These devices are not approved for residential installation.
- The drain lines for these devices shall terminate with acceptable air gaps that conform to ASME A112.1.2, or ASME A112.1.3.
- All piping between the outlets of these devices and the inlets of any downstream analyzers, and the water contacting materials of any downstream analyzers, shall be acceptable for contact with high purity water.
- Cross connection control is optional prior to these devices.
- Cross connection control, acceptable for high hazard, shall be installed downstream of these devices and prior to the analyzer being served. This is the responsibility of the owner of the analyzer.

The department is in no way endorsing this product or any advertising, and is not responsible for any situation which may result from its use.

Sincerely,

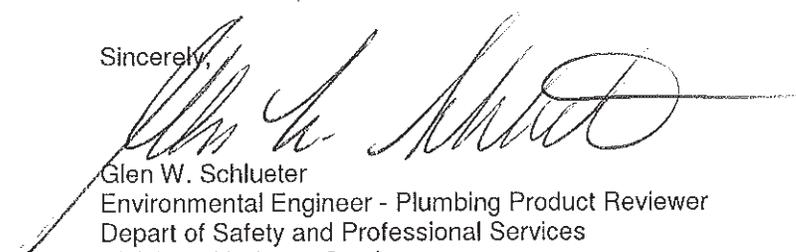

Glen W. Schlueter
Environmental Engineer - Plumbing Product Reviewer
Department of Safety and Professional Services
Division of Industry Services
Bureau of Technical Services
(608) 267-1401 Phone
(608) 267-9723 Fax
glen.schlueter@wi.gov E-mail